


Foshan Flying Medical Products Co., Ltd
CERTIFICATE OF STERILIZATION ANALYSIS

Manufacturer		Sleek Brows Ltd., for Everlasting Brows		Product Description		EVERLASTING BROWS DISPOSABLE TOOL	
Country of Manufactory		P.R.China		Expiration Date		26/07/2023	
Size		5*20		Lot Number		EVER040	
Item#		EL01		Inspection Date		10/08/2018	
PO#		PO:180525Z21		Customer Name		Everlasting Brows	
Flying PO#		PN:180525Z21		QTY		60000pcs	
NO	Test Item	Requirements	Inspection Standard	Inspected Qty.	Result	Conclusion	
1	Appearance	Clean, level off, no besmirch, no breakage	S-3	60000pcs	Accord	Pass	
2	Package Size	5CM*20CM Dialysis bag	S-2	60000pcs	Accord	Pass	
3	Box size	50cm*50cm*50cm			Accord	Pass	
4	Shear Strength	≥1N/cm			Accord	Pass	
5	Unwrap Quality	Good and ease to unwrap			Accord	Pass	
6	Seal	Sealed			Accord	Pass	
7	Printing Quality	Good quality good align				Pass	
8	Sterilization	Sterility	N/A	60000pcs	Accord	Pass	
Final Conclusion			Inspection Passed				

Drafted by
Date :10/08/2018 *Jane Zhang*

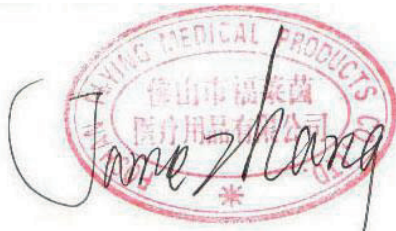

Approved by
Date :10/08/2018 *Jane Zhang*

Foshan Flying Medical Products Co., Ltd

Sterilization Inspection Report

NO :20180510003

PO	PO180525Z21			Product	EVERLASTING BROWS DISPOSABLE TOOL		
LOT	EVER040			Item#	EL01		
Sterilization Date	10/08/2018			Size	5*20		
Sterilization Lot	EVER030			Amount	60000pcs		
Process Parameter Summary				Inspection Basis	EN ISO 11737		
Temperature	50 ±2			Humidity	45-80%		
Exposure Time(h)	10h			EO Weight(kg)	480 kgs		
Biological Indicator Status							
Manufacture	Hangzhou Future			Organism	ATCC 9372		
Lot	20180603			D-value	3.5min		
Population	2.2*10 C.F.U			Test Quantity	10+1 strips		
Incubation Situation							
Incubation Date	2018.8.10-2018.8.17			Incubation Temperature	35±2		
Incubation Time	168			Medium Name	Soybean Casein Digest Medium		
Incubation Time	After 24h	After 48h	After 72h	After 96h	After 120h	After 144h	After 168h
Observed Item	(-)	(-)	(-)	(-)	(-)	(-)	(-)
Positive Control	(+)						
<p>Conclusion : Qualified</p> <p>Qualified</p> <p>Sterilized by EO,the products comply with ISO 11737 standard(Sterilization of medical devices--Microbiological methods--Part2:Tests of sterility performed in the validation of a sterilization process).</p>							

Note

(-) represent of negative BI,no bacterial growth

(+) represent of negative BI,bacterial growth

Drafted by Jane Zhang

Approved by Jane Zhang

Date:17/08/2018

Date : 17/08/2018

